

1 / 6

Fig. 1


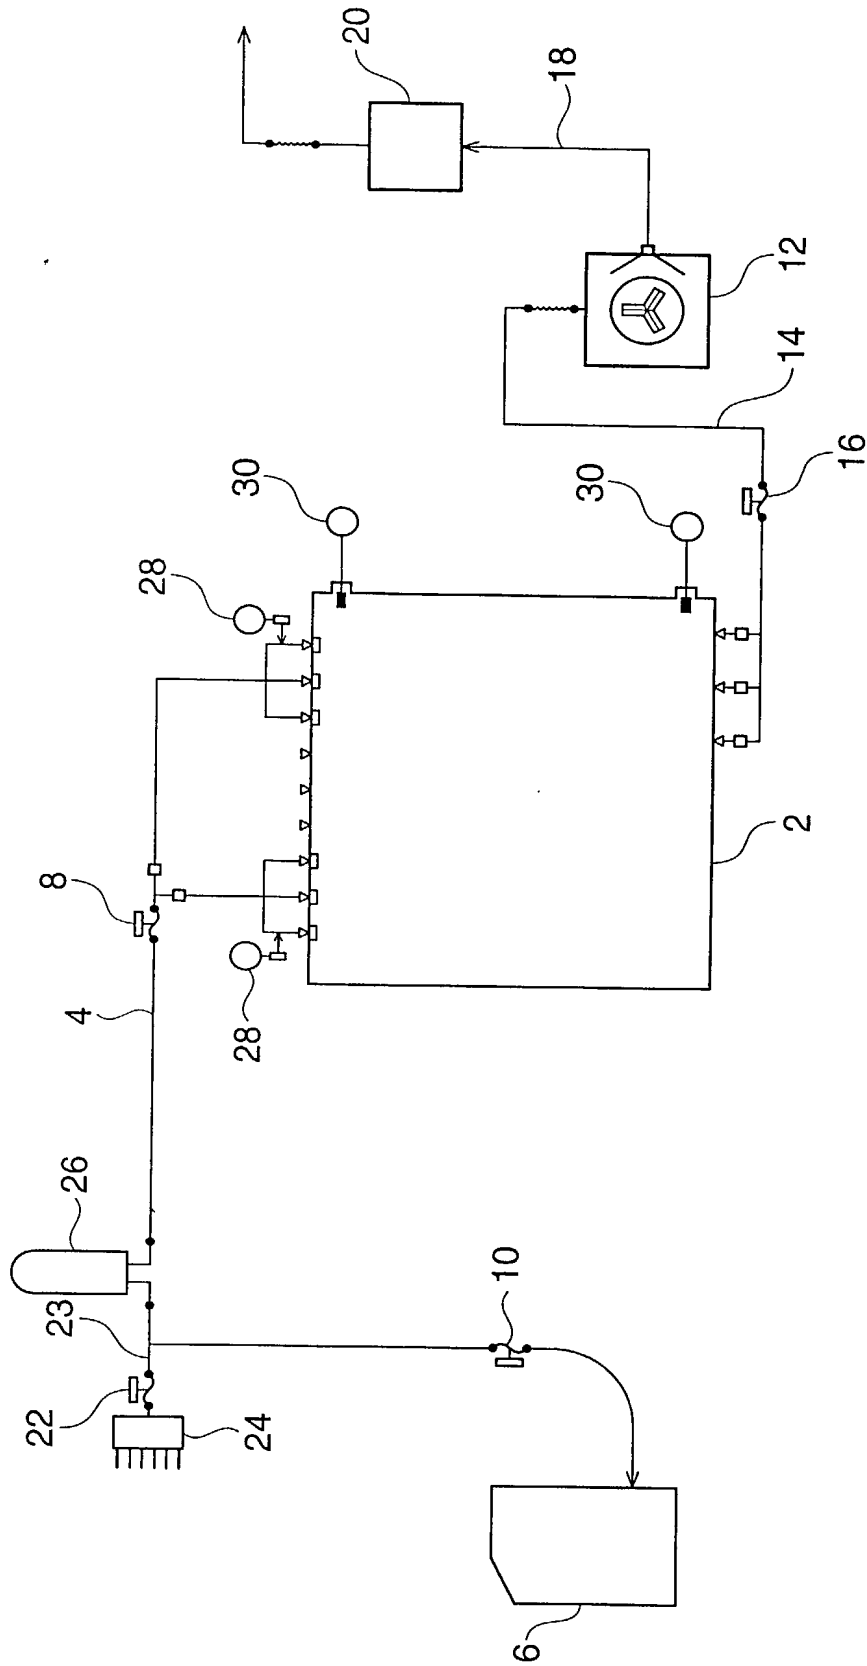


Fig. 2


Outlined Process for Sterilization Cycle

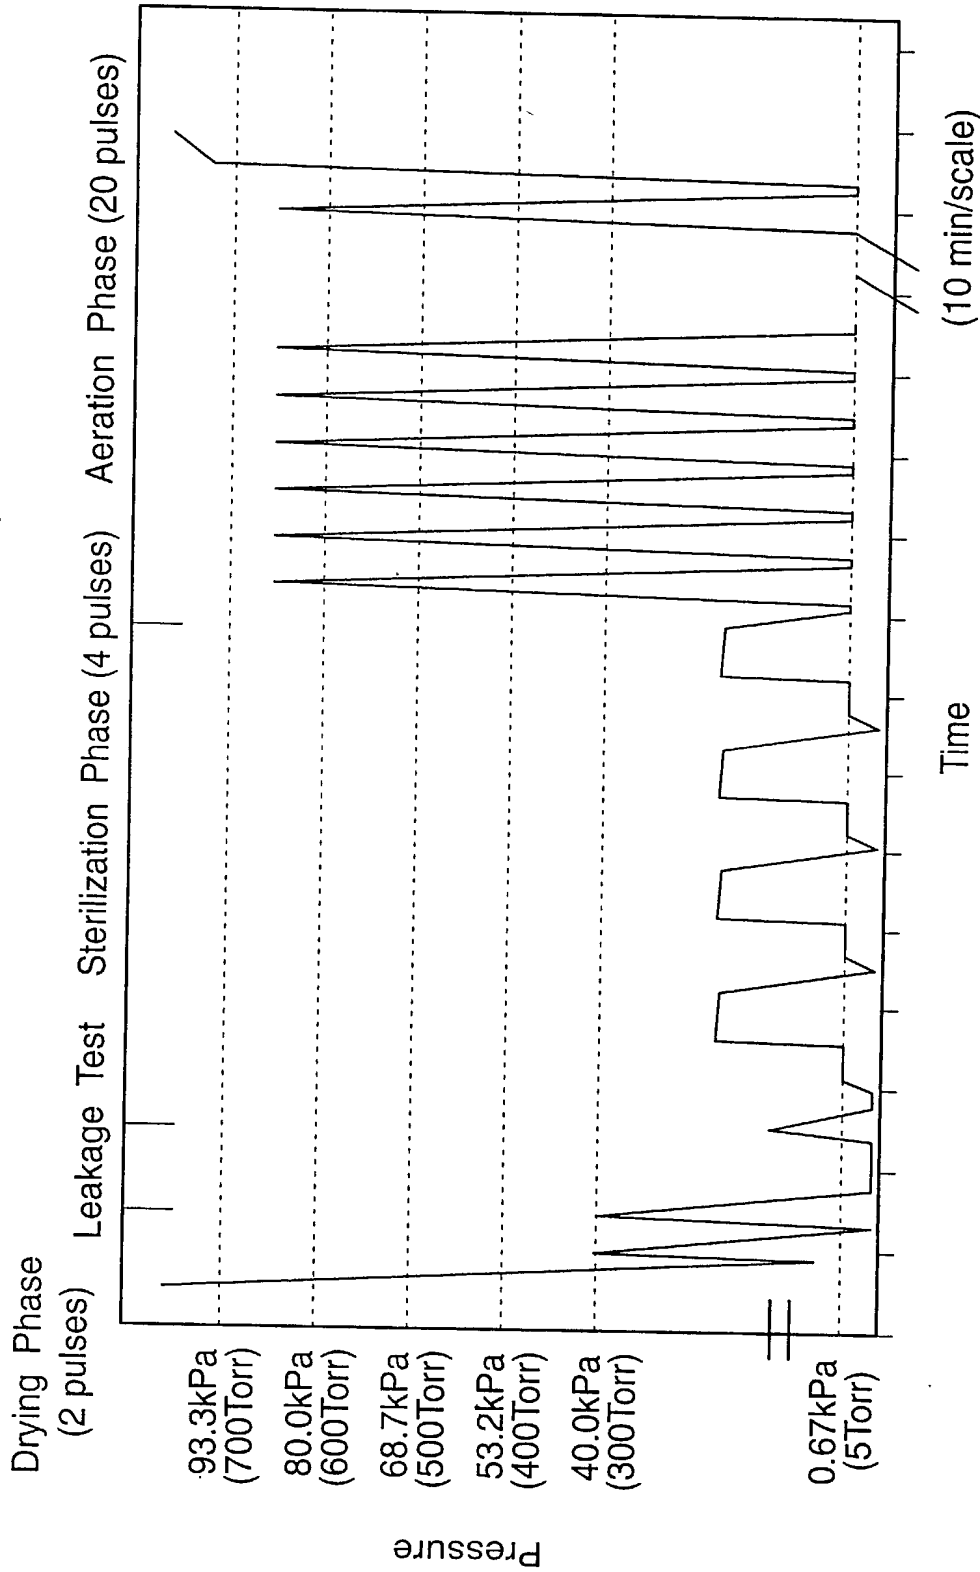

In case where the sterilization cycle comprises a combination of 4 pulses of gaseous hydrogen peroxide treatment and 20 aeration pulses, the sterilization process requires about 3 hours and 20 minutes.


Fig. 3

Correlation between the storage time and the residual hydrogen peroxide concentration

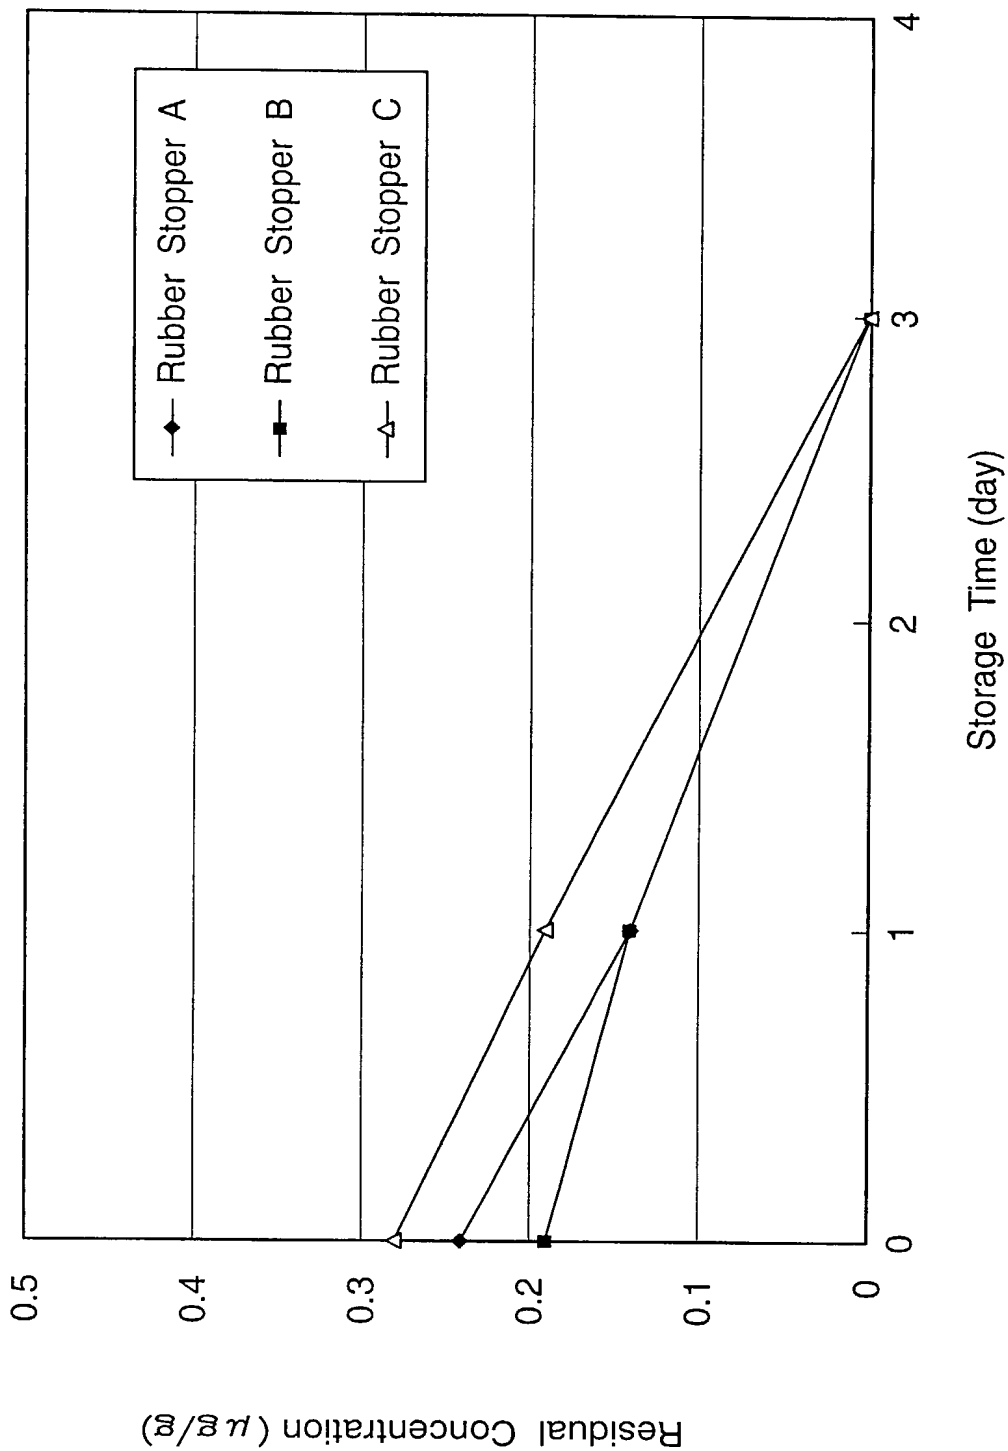


4/6

Fig. 4

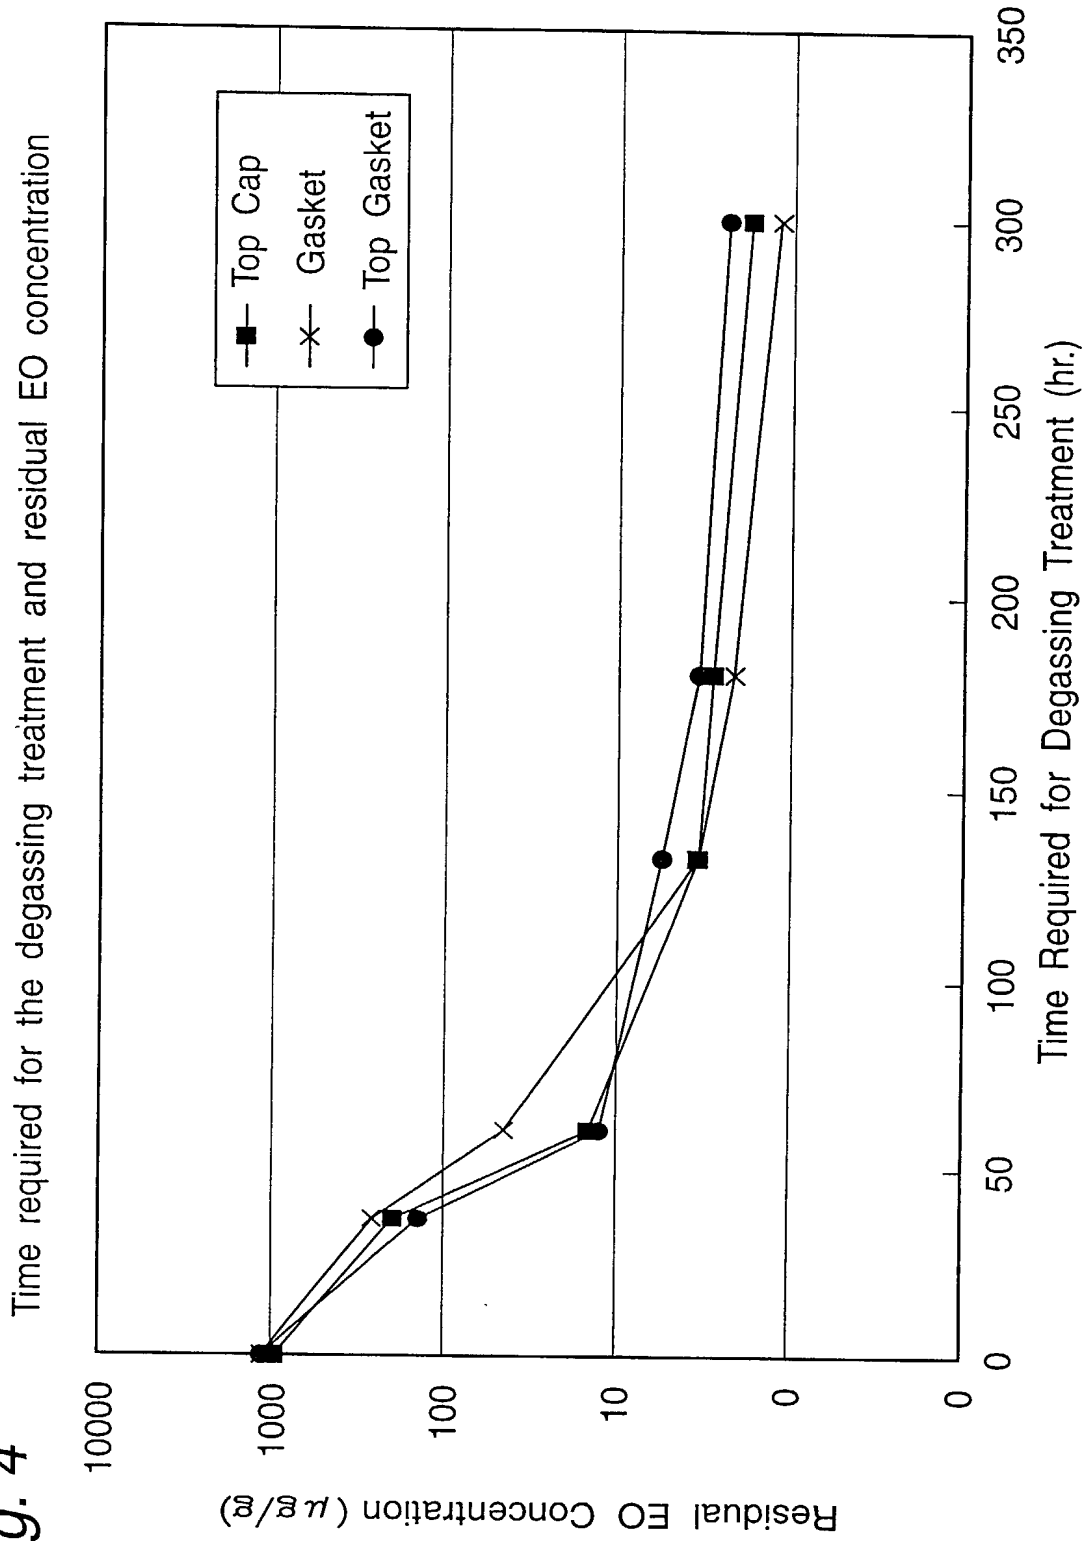

5/6

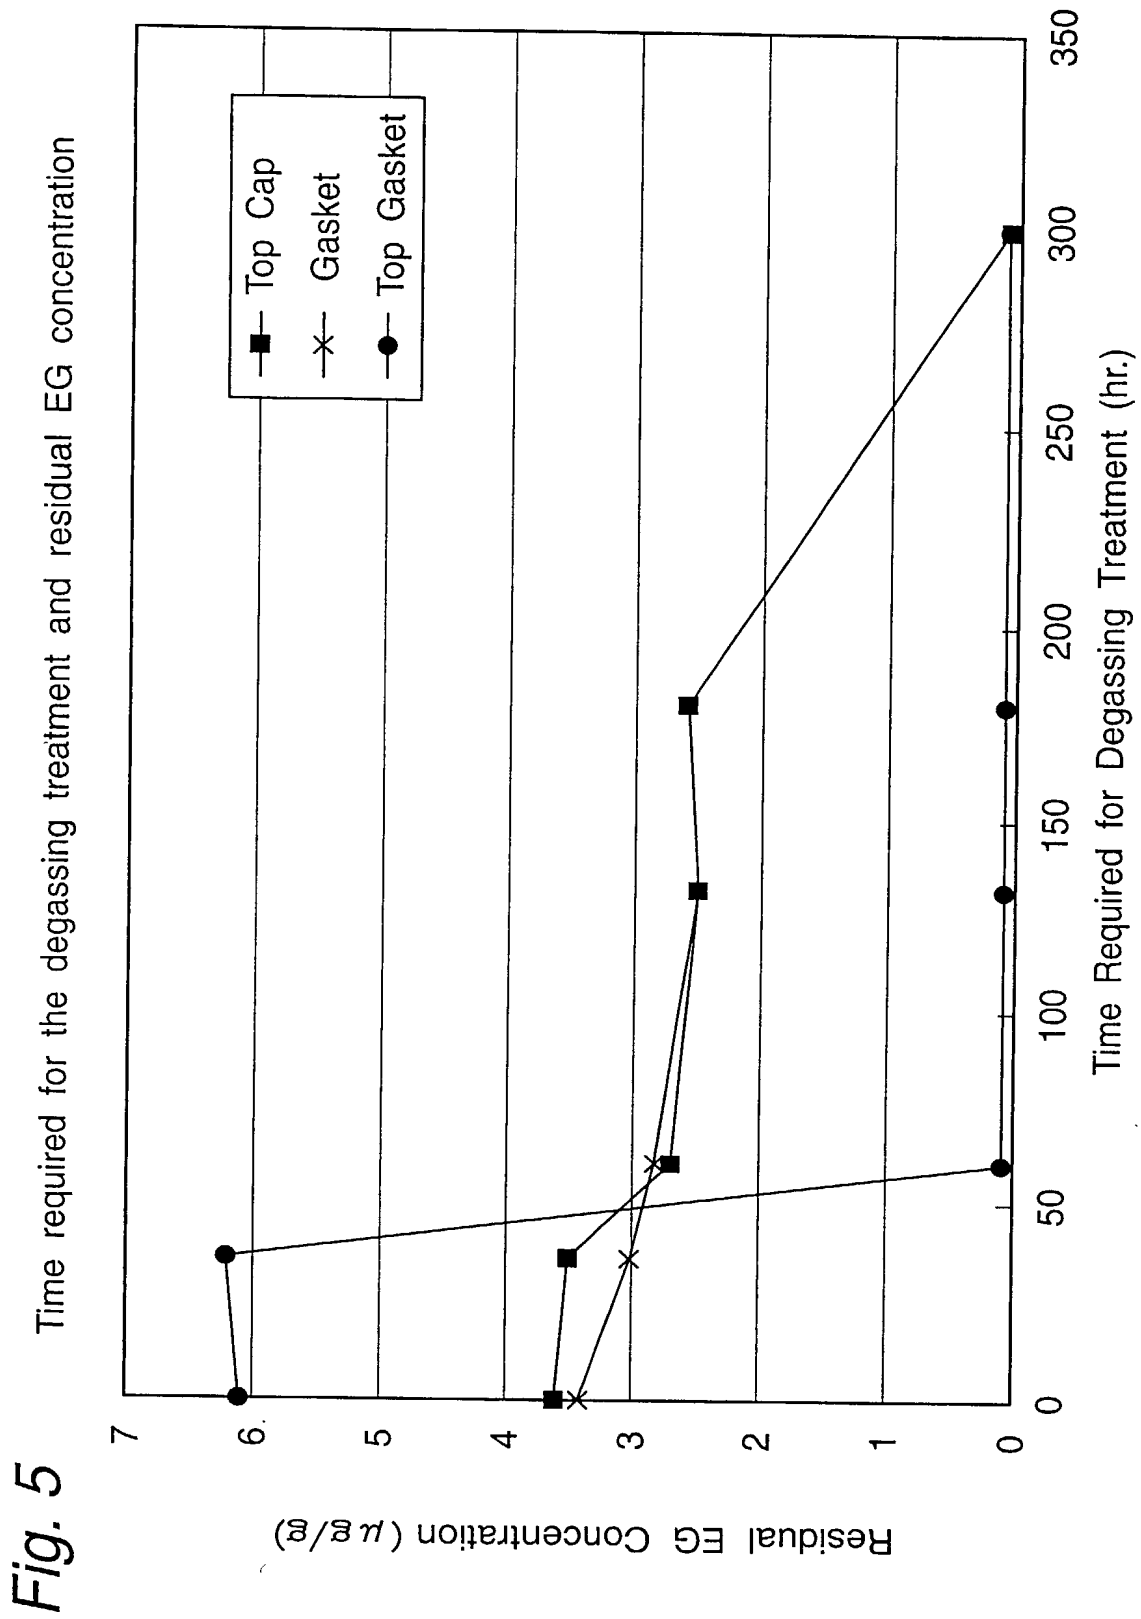

6/6

Fig. 6

